


# FOR FAECAL CONCENTRATION OF

HELMINTH OVA AND LARVAE / PROTOZOA CYSTS AND OOCYSTS

APACOR

Mini Parasep® SF  
FAECAL PARASITE CONCENTRATOR

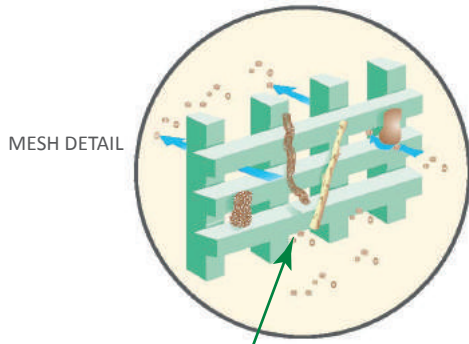

SELF STANDING  
SAMPLE CHAMBER

MIXING CHAMBER

INTEGRAL  
SPOON

#### Filter

A two stage filtration matrix. Large particles are rejected without occluding the 425µm pores. Recovery rate with Parasep® is comparable to traditional sieve method, ie: Ridley-Allen. The vertical filter enclosed design is patented.

#### Debris Trap

Rejected particles are trapped to prevent extrusion into the Sedimentation Cone during centrifugation.

#### Air/Liquid Seal and Safety Lock

The 'seal' prevents the release of biohazardous material. The 'lock' ensures the Mixing Chamber and Filter are removed together for safe disposal.

#### Fat Dispersion Chamber

A perforated fat dispersion chamber removes the smaller faecal debris and separates the fat content so that it can be efficiently removed from the resulting sediment without the use of ether or ethyl acetate.

#### Sedimentation Cone

Sediment forms in the base of the cone allowing examination for the presence of helminth eggs or larvae and protozoa cysts or oocysts.

#### Health and Safety Benefits

- Totally enclosed/sealed process
- Reduced reagent volumes
- No cleaning required
- Single use, no sample contamination
- Ready to use systems available

#### Performance Benefits

- Optimum sample recovery
- Enhanced sample clarity
- Rapid four step process
- Human resources optimised
- Easy patient identification
- Fits all 15ml centrifuge buckets



## PARASITOLOGY

SINGLE USE IN VITRO DIAGNOSTIC DEVICE



# Procedure

## STEP 1 - SAMPLE PREPARATION

### Preserved Samples

Shake or vortex the incoming preserved sample to thoroughly mix.

Transfer either 2ml (**US Gold Standard**) or 3ml (**ARUP JCM**) of the emulsified stool into the Mini Parasep® SF mixing chamber.

In the event of:

**Thick Stool Samples**—please add 10 drops of Apacor Triton X, then please enclose and vortex/shake to emulsify prior to transferring the sample;

**Liquid Stool Samples**—please add 4ml instead of 2ml or 3ml to ensure that a sediment is formed after centrifugation is performed.



## STEP 2 - EMULSIFICATION

Seal the Mini Parasep® SF by screwing in the filter/sedimentation cone unit.



## STEP 3 - CENTRIFUGATION

Invert Mini Parasep® SF and perform centrifugation at:


**500g** for ten minutes (**US Gold Standard**);

**400g** for two minutes (**ARUP JCM**).

NOTE: TO CALCULATE THE REQUIRED RPM FOR ANY CENTRIFUGE.

$$RPM = \sqrt{\frac{g}{1.12r}} \times 1000$$

RPM - rotor speed in revs/min.  
g - centrifugal force (max. 1000g)  
r - radius, horizontal distance between sedimentation cone tip and spindle centre measured in mm.

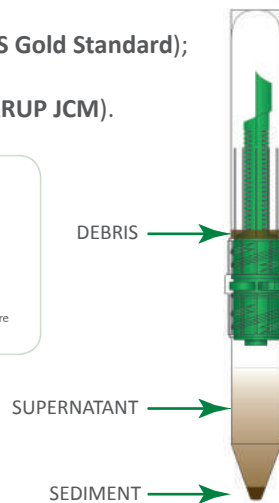


## STEP 4 - EXAMINATION

Unscrew and discard the filter and mixing tube.

Decant the supernatant.

Transfer sediment to slide to perform examination where all temporary (Lugol's Iodine) and permanent staining techniques (Trichrome) can be conducted providing a universal fixative is used.

If a universal fixative is used in conjunction with this device, then molecular and EIA tests can be conducted from the sediment.



See label for storage conditions and expiry date. Please adhere to the following guidelines when handling Mini Parasep® SF. To avoid cross contamination the Mini Parasep® SF device should remain closed at all times except when introducing the sample or when retrieving the final concentrated sample for examination.

**Mini Parasep® SF is available empty or reagent ready**  
**Please ask for details**

Products can be ordered direct from Apacor or from an appointed distributor  
Visit our website for all the latest information [www.apacor.com](http://www.apacor.com) or email on: [sales@apacor.com](mailto:sales@apacor.com)



UNIT 5 SAPPHIRE CENTRE  
FISHPONDS ROAD, WOKINGHAM  
BERKSHIRE, RG41 2QL, ENGLAND  
TEL: +44 (0)118 979 5566  
FAX: +44 (0)118 979 5186

